


Operator: John Doe  
Process: Lyo  
Session Start: 2008-05-12 3:00:00 PM  
Session Stop: 2008-05-19 3:54:00 PM  
Session Name: Demo  
Session Text: Qualification

Vessel: Lyophil 550  
Product: Pharma  
Time Zone: Pacific Daylight Time (UTC offset - 07:00:00)




### Statistics

#### Graphic Representation Min



#### Graphic Representation Max




Operator/Date:

Operator: John Doe  
Process: Lyo  
Session Start: 2008-05-12 3:00:00 PM  
Session Stop: 2008-05-19 3:54:00 PM  
Session Name: Demo  
Session Text: Qualification


Vessel: Lyophil 550  
Product: Pharma  
Time Zone: Pacific Daylight Time (UTC offset - 07:00:00)



### Graphic Representation Average

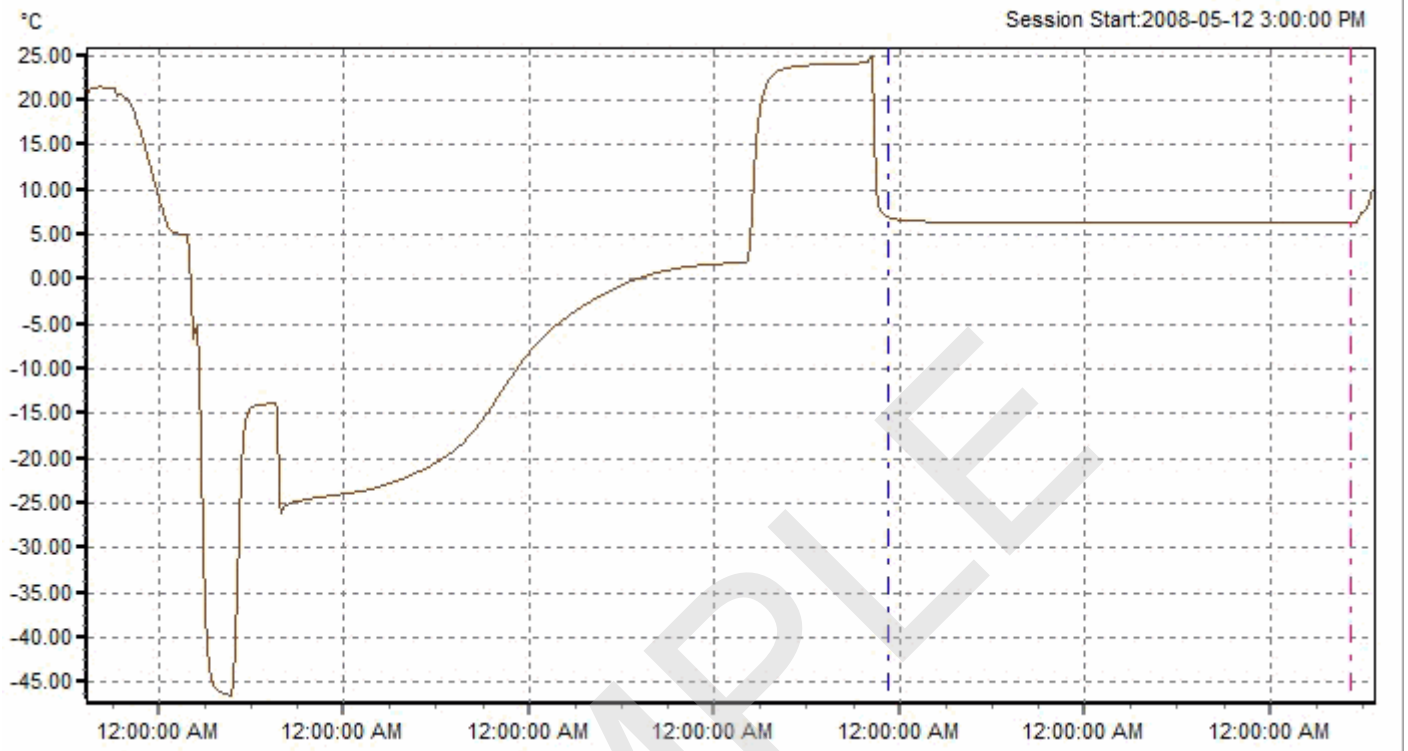

### Graphic Representation Delta




Operator/Date:

Operator: John Doe  
Process: Lyo  
Session Start: 2008-05-12 3:00:00 PM  
Session Stop: 2008-05-19 3:54:00 PM  
Session Name: Demo  
Session Text: Qualification


Vessel: Lyophil 550  
Product: Pharma  
Time Zone: Pacific Daylight Time (UTC offset - 07:00:00)



### Graphic Representation Standard Deviation



### Graphic Representation Max Minus Average




Operator/Date:

Operator: John Doe  
 Process: Lyo  
 Session Start: 2008-05-12 3:00:00 PM  
 Session Stop: 2008-05-19 3:54:00 PM  
 Session Name: Demo  
 Session Text: Qualification

Vessel: Lyophil 550  
 Product: Pharma  
 Time Zone: Pacific Daylight Time (UTC offset - 07:00:00)



Graphic Representation Average Minus Min.



Name	Statistics
Description	Temperature
Type	Temperature
Start Time	2008-05-12 3:00:00 PM
Stop Time	2008-05-19 3:54:00 PM
Global Min.	-50.04 °C
Global Max.	31.15 °C
Global Average	-0.02 °C
Min average	-2.30 °C
Max average	2.29 °C
Global Delta	81.19 °C
Global Standard Deviation	15.53 °C
Global Max. Minus	31.18 °C
Global Average Minus	50.01 °C

- 2008-05-13 9:08:00 AM LC 11
- 2008-05-13 9:10:00 AM LC 11
- 2008-05-13 9:11:00 AM LC 11
- 2008-05-13 9:12:00 AM LC 11
- 2008-05-13 9:13:00 AM LC 11
- 2008-05-13 9:14:00 AM LC 11
- 2008-05-13 9:15:00 AM LC 11
- 2008-05-13 9:16:00 AM LC 11
- 2008-05-13 9:17:00 AM LC 11
- 2008-05-13 9:18:00 AM LC 11
- 2008-05-13 9:19:00 AM LC 11
- 2008-05-13 9:20:00 AM LC 11
- 2008-05-13 9:21:00 AM LC 11
- 2008-05-12 10:25:00 PM LA 40

LC 67  
 LA 48

ID	Name	Description	Min.	Max.	Average	Delta	Standard Deviation
			Max. - Avg.	Avg. - Min.			

Operator/Date:

Operator: John Doe  
 Process: Lyo  
 Session Start: 2008-05-12 3:00:00 PM  
 Session Stop: 2008-05-19 3:54:00 PM  
 Session Name: Demo  
 Session Text: Qualification

Vessel: Lyophil 550  
 Product: Pharma  
 Time Zone: Pacific Daylight Time (UTC offset - 07:00:00)



23783-2	LA 10	Temperature	-45.30 °C	27.99 °C	0.71 °C	73.29 °C	14.82 °C
			27.28 °C	46.01 °C			
23760-2	LA 12	Temperature	-49.25 °C	26.88 °C	0.39 °C	76.13 °C	14.88 °C
			26.49 °C	49.64 °C			
23786-2	LA 14	Temperature	-44.99 °C	24.48 °C	1.14 °C	69.47 °C	14.27 °C
			23.34 °C	46.12 °C			
23814-2	LA 16	Temperature	-46.13 °C	24.99 °C	0.76 °C	71.12 °C	15.10 °C
			24.24 °C	46.89 °C			
23731-2	LA 18	Temperature	-43.63 °C	24.76 °C	0.97 °C	68.39 °C	15.00 °C
			23.79 °C	44.59 °C			
23812-2	LA 2	Temperature	-45.79 °C	24.40 °C	1.65 °C	70.19 °C	14.26 °C
			22.75 °C	47.43 °C			
23757-2	LA 20	Temperature	-45.32 °C	24.08 °C	1.38 °C	69.40 °C	13.76 °C
			22.70 °C	46.70 °C			
23809-2	LA 22	Temperature	-45.86 °C	25.70 °C	0.43 °C	71.56 °C	15.13 °C
			25.27 °C	46.28 °C			
23785-2	LA 24	Temperature	-47.24 °C	24.63 °C	-0.05 °C	71.87 °C	15.64 °C
			24.68 °C	47.19 °C			
23791-2	LA 26	Temperature	-45.83 °C	24.95 °C	0.16 °C	70.78 °C	15.56 °C
			24.79 °C	45.99 °C			
23795-2	LA 28	Temperature	-43.77 °C	24.76 °C	-0.11 °C	68.53 °C	15.48 °C
			24.87 °C	43.65 °C			
23756-2	LA 30	Temperature	-42.80 °C	24.72 °C	0.24 °C	67.52 °C	15.35 °C
			24.47 °C	43.04 °C			
23804-2	LA 32	Temperature	-47.29 °C	24.79 °C	0.98 °C	72.08 °C	15.00 °C
			23.81 °C	48.27 °C			
23790-2	LA 34	Temperature	-45.32 °C	24.59 °C	1.61 °C	69.91 °C	14.28 °C
			22.98 °C	46.93 °C			
23799-2	LA 36	Temperature	-45.52 °C	24.72 °C	0.51 °C	70.24 °C	15.16 °C
			24.21 °C	46.03 °C			
23787-2	LA 38	Temperature	-42.09 °C	24.67 °C	0.49 °C	66.76 °C	15.05 °C
			24.18 °C	42.59 °C			
23797-2	LA 4	Temperature	-45.82 °C	24.71 °C	0.90 °C	70.53 °C	14.76 °C
			23.80 °C	46.72 °C			
23808-2	LA 40	Temperature	-48.36 °C	31.15 °C	0.44 °C	79.51 °C	14.91 °C
			30.72 °C	48.80 °C			
23813-2	LA 42	Temperature	-48.76 °C	27.62 °C	0.73 °C	76.38 °C	15.04 °C
			26.89 °C	49.49 °C			
23781-2	LA 44	Temperature	-44.92 °C	24.55 °C	1.87 °C	69.47 °C	14.55 °C
			22.68 °C	46.79 °C			
23794-2	LA 46	Temperature	-47.64 °C	24.55 °C	0.46 °C	72.19 °C	15.38 °C
			24.09 °C	48.10 °C			
23802-2	LA 48	Temperature	-43.66 °C	24.61 °C	2.29 °C	68.27 °C	14.31 °C
			22.32 °C	45.95 °C			
23768-2	LA 50	Temperature	-43.64 °C	24.30 °C	0.91 °C	67.94 °C	14.52 °C
			23.39 °C	44.55 °C			
23764-2	LA 52	Temperature	-42.09 °C	24.83 °C	0.06 °C	66.92 °C	15.36 °C
			24.77 °C	42.15 °C			
23811-2	LA 54	Temperature	-43.49 °C	27.24 °C	1.60 °C	70.73 °C	14.06 °C
			25.64 °C	45.10 °C			
23767-2	LA 56	Temperature	-49.73 °C	25.54 °C	0.46 °C	75.27 °C	14.42 °C
			25.08 °C	50.19 °C			
23761-2	LA 58	Temperature	-44.86 °C	24.50 °C	1.69 °C	69.36 °C	13.92 °C
			22.81 °C	46.55 °C			

Operator/Date:

Operator: John Doe  
 Process: Lyo  
 Session Start: 2008-05-12 3:00:00 PM  
 Session Stop: 2008-05-19 3:54:00 PM  
 Session Name: Demo  
 Session Text: Qualification

Vessel: Lyophil 550  
 Product: Pharma  
 Time Zone: Pacific Daylight Time (UTC offset - 07:00:00)



23807-2	LA 6	Temperature	-44.95 °C	24.89 °C	0.67 °C	69.84 °C	15.14 °C
			24.21 °C	45.62 °C			
23780-2	LA 60	Temperature	-49.85 °C	25.51 °C	0.85 °C	75.36 °C	14.19 °C
			24.66 °C	50.70 °C			
23762-2	LA 62	Temperature	-40.88 °C	24.60 °C	-0.66 °C	65.48 °C	15.31 °C
			25.26 °C	40.23 °C			
23769-2	LA 64	Temperature	-44.23 °C	25.30 °C	1.52 °C	69.53 °C	14.20 °C
			23.78 °C	45.76 °C			
23788-2	LA 66	Temperature	-42.10 °C	24.69 °C	1.48 °C	66.79 °C	14.00 °C
			23.21 °C	43.58 °C			
23775-2	LA 68	Temperature	-49.33 °C	25.68 °C	-0.26 °C	75.01 °C	14.82 °C
			25.95 °C	49.07 °C			
23810-2	LA 70	Temperature	-46.33 °C	24.94 °C	-0.72 °C	71.27 °C	15.94 °C
			25.66 °C	45.60 °C			
23759-2	LA 72	Temperature	-41.80 °C	24.97 °C	0.79 °C	66.77 °C	14.19 °C
			24.18 °C	42.59 °C			
23806-2	LA 74	Temperature	-40.74 °C	29.71 °C	-0.22 °C	70.45 °C	15.21 °C
			29.94 °C	40.52 °C			
23770-2	LA 76	Temperature	-38.30 °C	24.55 °C	0.36 °C	62.85 °C	15.01 °C
			24.19 °C	38.66 °C			
23798-2	LA 78	Temperature	-42.94 °C	24.62 °C	1.27 °C	67.56 °C	14.68 °C
			23.35 °C	44.21 °C			
23771-2	LA 8	Temperature	-43.75 °C	24.68 °C	1.20 °C	68.43 °C	14.89 °C
			23.48 °C	44.95 °C			
23885-2	LA 80	Temperature	-49.80 °C	25.48 °C	-0.08 °C	75.28 °C	14.91 °C
			25.56 °C	49.73 °C			
23812-1	LC 1	Temperature	-48.68 °C	24.90 °C	-0.87 °C	73.58 °C	16.17 °C
			25.77 °C	47.81 °C			
23760-1	LC 11	Temperature	-50.04 °C	25.55 °C	-1.34 °C	75.59 °C	16.31 °C
			26.90 °C	48.69 °C			
23786-1	LC 13	Temperature	-48.44 °C	24.86 °C	-0.69 °C	73.30 °C	16.00 °C
			25.55 °C	47.75 °C			
23814-1	LC 15	Temperature	-46.77 °C	25.14 °C	-0.61 °C	71.91 °C	16.27 °C
			25.75 °C	46.16 °C			
23731-1	LC 17	Temperature	-47.87 °C	25.07 °C	0.21 °C	72.94 °C	15.76 °C
			24.86 °C	48.08 °C			
23757-1	LC 19	Temperature	-48.91 °C	23.72 °C	0.20 °C	72.63 °C	14.07 °C
			23.53 °C	49.11 °C			
23809-1	LC 21	Temperature	-49.74 °C	25.52 °C	-0.56 °C	75.26 °C	16.04 °C
			26.08 °C	49.19 °C			
23785-1	LC 23	Temperature	-49.25 °C	24.99 °C	-1.32 °C	74.24 °C	16.62 °C
			26.32 °C	47.93 °C			
23791-1	LC 25	Temperature	-47.71 °C	25.16 °C	-1.00 °C	72.87 °C	16.39 °C
			26.17 °C	46.71 °C			
23795-1	LC 27	Temperature	-47.21 °C	24.86 °C	-1.34 °C	72.07 °C	16.91 °C
			26.20 °C	45.87 °C			
23756-1	LC 29	Temperature	-47.34 °C	25.07 °C	-0.91 °C	72.41 °C	16.45 °C
			25.98 °C	46.43 °C			
23797-1	LC 3	Temperature	-47.96 °C	25.03 °C	-0.65 °C	72.99 °C	16.25 °C
			25.68 °C	47.31 °C			
23804-1	LC 31	Temperature	-48.93 °C	25.08 °C	-0.91 °C	74.01 °C	16.66 °C
			25.99 °C	48.02 °C			
23790-1	LC 33	Temperature	-46.96 °C	24.79 °C	-0.34 °C	71.75 °C	15.87 °C
			25.13 °C	46.62 °C			

Operator/Date:

Operator: John Doe  
 Process: Lyo  
 Session Start: 2008-05-12 3:00:00 PM  
 Session Stop: 2008-05-19 3:54:00 PM  
 Session Name: Demo  
 Session Text: Qualification

Vessel: Lyophil 550  
 Product: Pharma  
 Time Zone: Pacific Daylight Time (UTC offset - 07:00:00)



23799-1	LC 35	Temperature	-47.96 °C	25.06 °C	-1.67 °C	73.02 °C	16.86 °C
			26.74 °C	46.28 °C			
23787-1	LC 37	Temperature	-45.47 °C	24.95 °C	-1.26 °C	70.42 °C	16.64 °C
			26.21 °C	44.21 °C			
23808-1	LC 39	Temperature	-49.97 °C	25.51 °C	-1.96 °C	75.48 °C	16.97 °C
			27.47 °C	48.01 °C			
23813-1	LC 41	Temperature	-49.67 °C	25.57 °C	-0.64 °C	75.24 °C	16.18 °C
			26.21 °C	49.03 °C			
23781-1	LC 43	Temperature	-47.47 °C	24.88 °C	0.18 °C	72.35 °C	16.11 °C
			24.70 °C	47.66 °C			
23794-1	LC 45	Temperature	-49.38 °C	24.95 °C	-0.83 °C	74.33 °C	16.32 °C
			25.78 °C	48.56 °C			
23802-1	LC 47	Temperature	-47.82 °C	25.01 °C	0.42 °C	72.83 °C	16.07 °C
			24.59 °C	48.24 °C			
23768-1	LC 49	Temperature	-48.06 °C	24.81 °C	-1.14 °C	72.87 °C	16.12 °C
			25.95 °C	46.92 °C			
23807-1	LC 5	Temperature	-47.70 °C	25.13 °C	0.00 °C	72.83 °C	15.75 °C
			25.12 °C	47.70 °C			
23764-1	LC 51	Temperature	-47.36 °C	25.14 °C	-0.81 °C	72.50 °C	16.19 °C
			25.95 °C	46.54 °C			
23811-1	LC 53	Temperature	-48.12 °C	25.30 °C	-0.74 °C	73.42 °C	16.03 °C
			26.04 °C	47.39 °C			
23767-1	LC 55	Temperature	-49.92 °C	25.52 °C	-1.41 °C	75.44 °C	16.20 °C
			26.93 °C	48.51 °C			
23761-1	LC 57	Temperature	-48.44 °C	25.01 °C	-1.66 °C	73.45 °C	16.40 °C
			26.67 °C	46.78 °C			
23780-1	LC 59	Temperature	-50.00 °C	25.52 °C	-1.22 °C	75.52 °C	16.22 °C
			26.74 °C	48.78 °C			
23762-1	LC 61	Temperature	-47.23 °C	24.97 °C	-1.11 °C	72.20 °C	16.04 °C
			26.08 °C	46.13 °C			
23769-1	LC 63	Temperature	-47.55 °C	25.17 °C	-0.35 °C	72.72 °C	15.88 °C
			25.51 °C	47.21 °C			
23788-1	LC 65	Temperature	-46.29 °C	24.98 °C	-0.07 °C	71.27 °C	15.47 °C
			25.05 °C	46.22 °C			
23775-1	LC 67	Temperature	-49.87 °C	25.54 °C	-2.30 °C	75.41 °C	16.61 °C
			27.84 °C	47.57 °C			
23810-1	LC 69	Temperature	-43.10 °C	24.66 °C	0.58 °C	67.76 °C	14.87 °C
			24.08 °C	43.68 °C			
23771-1	LC 7	Temperature	-47.03 °C	25.00 °C	-0.77 °C	72.03 °C	16.53 °C
			25.77 °C	46.26 °C			
23759-1	LC 71	Temperature	-46.68 °C	24.65 °C	-0.43 °C	71.33 °C	15.49 °C
			25.08 °C	46.25 °C			
23806-1	LC 73	Temperature	-46.17 °C	25.03 °C	0.45 °C	71.20 °C	14.75 °C
			24.58 °C	46.62 °C			
23770-1	LC 75	Temperature	-46.28 °C	25.03 °C	-1.07 °C	71.31 °C	16.22 °C
			26.10 °C	45.21 °C			
23798-1	LC 77	Temperature	-45.88 °C	24.97 °C	-1.27 °C	70.85 °C	16.31 °C
			26.24 °C	44.61 °C			
23885-1	LC 79	Temperature	-49.88 °C	25.53 °C	-2.00 °C	75.41 °C	16.52 °C
			27.53 °C	47.88 °C			
23783-1	LC 9	Temperature	-46.73 °C	24.93 °C	0.61 °C	71.66 °C	14.76 °C
			24.32 °C	47.34 °C			

Operator/Date: