
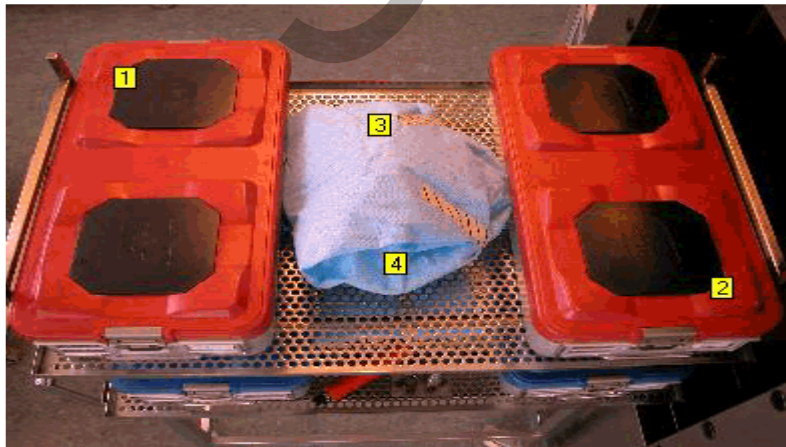


Operator: Validation mgr.
Process: Sterilisation
Session Start:
Session Stop:
Session Name: 11082008 Unit 1
Session Text: Periodic validation of sterilisation process

Vessel: Autoclave # 1
Product: Utensils
Time Zone: Rom, normaltid (UTC offset 02:00:00)

Unit Configuration:

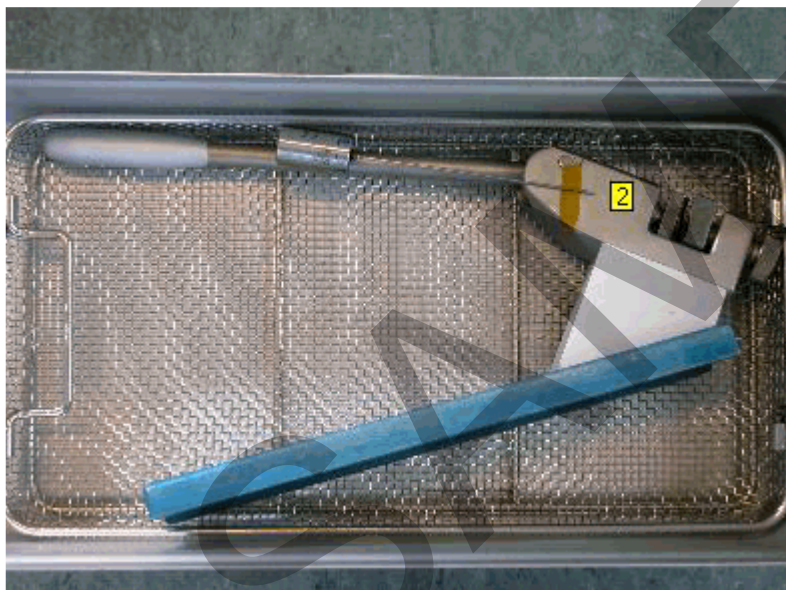

Operator: Validation mgr. Vessel: Autoclave # 1
Process: Sterilisation Product: Utensils
Session Start: Time Zone: Rom, normaltid (UTC offset 02:00:00)
Session Stop:
Session Name: 11082008 Unit 1
Session Text: Periodic validation of sterilisation process



Position 1: None Position 2: None Position 3: None Position 4: None Position 5: None
Position 6: None Position 7: None Position 8: None
Lethality N/A
Auto Start/Stop N/A

